
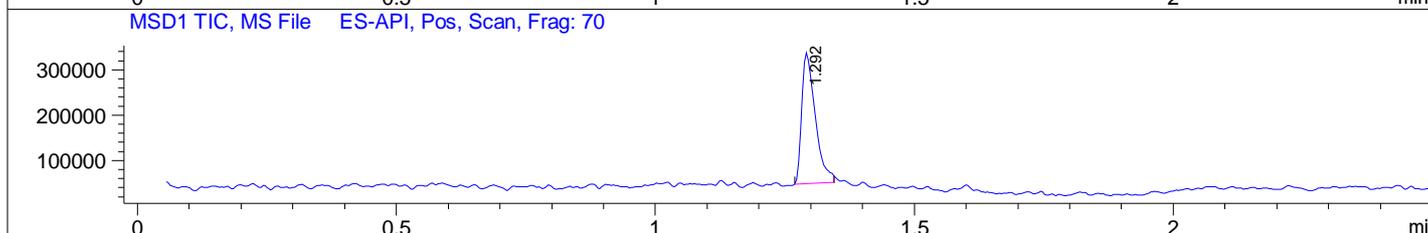
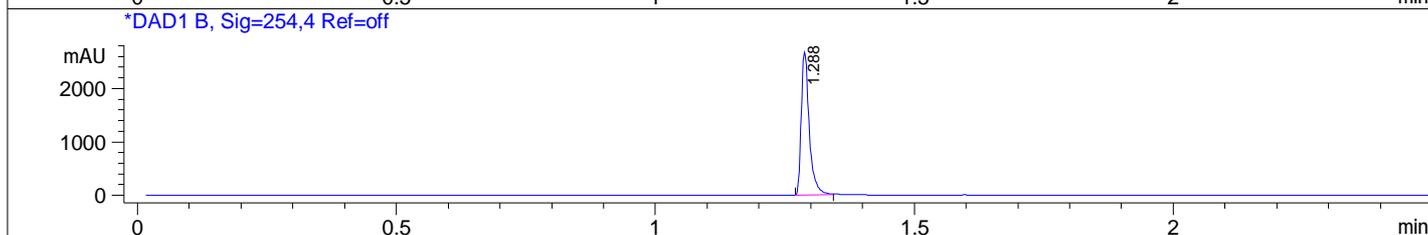
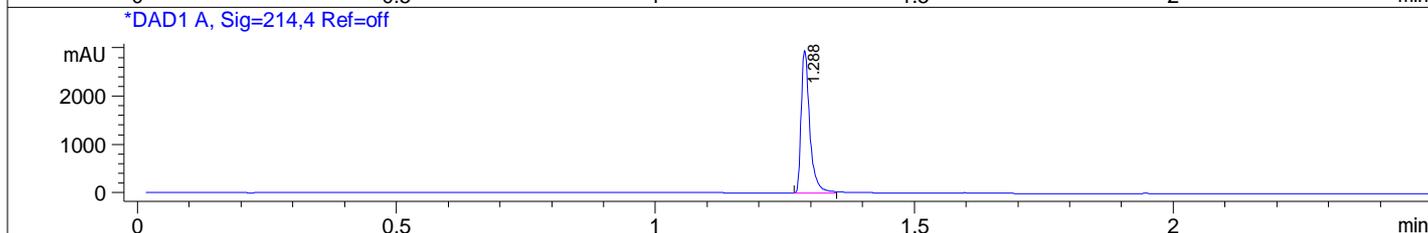


File D:\DATA\  
 Injection Date : 6 Mar 15 12:30 pm +0800 Tgt Mass (EZX) :  
 Sample Name : 530 Location : P2-A-05  
 Acq. Operator : LCMS Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\METHODS\1-POS-3MIN.M  
 Analysis Method : D:\METHODS\1-POS-3MIN.M  
 Sample Info : \*\*\* No target masses specified \*\*\*  
 Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)  
 Gradient: 5%-95% B in 1.2min  
 Flow Rate: 2.2 ml/min  
 Column: Poroshell 120 EC-C18,4.6\*30mm,2.7um  
 Oven Temperature: 50 C  
 Mass Range: 110-1500

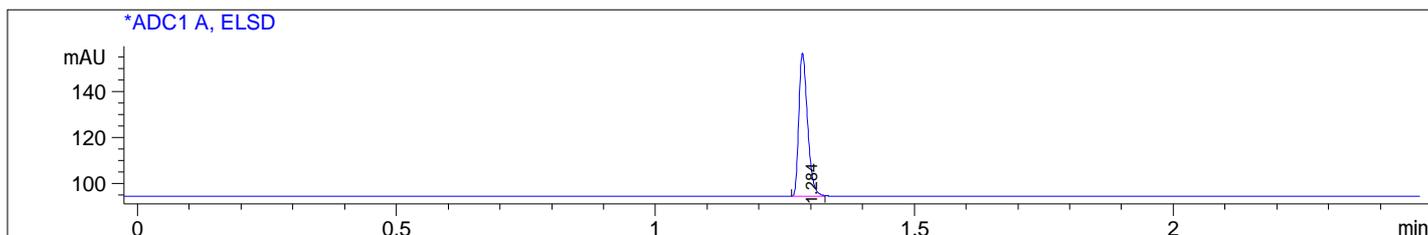

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.28	0.02	73.36	62.26	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.29	0.02	3343.69	2882.68	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.29	0.02	2816.85	2686.43	100.00

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

